
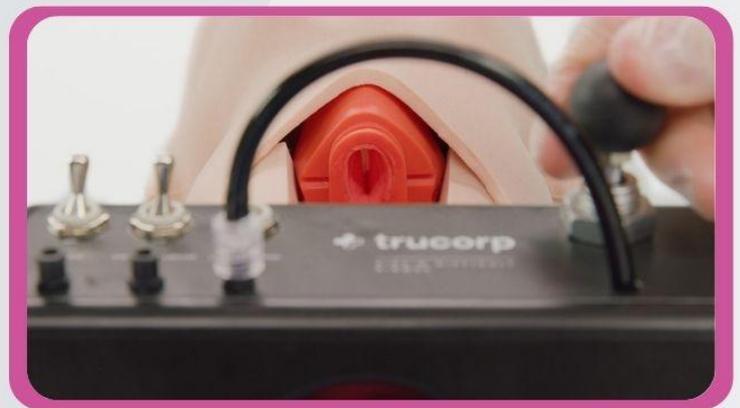


# AirSim Difficult Airway User Manual

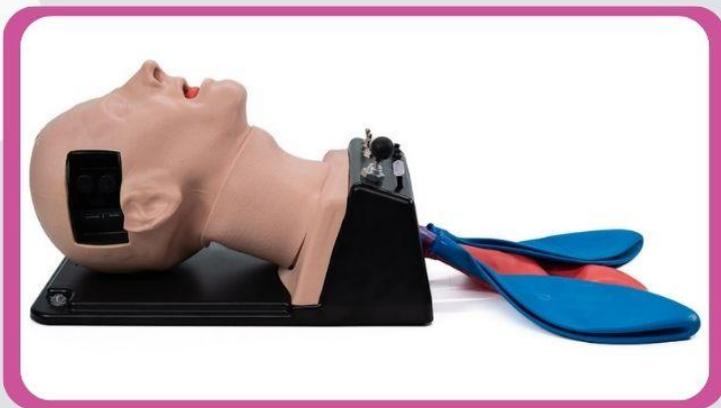

The AirSim Difficult Airway provides a solution for varying degrees of difficulty when practicing airway management.

This versatile model ranges from challenging to very difficult to intubate, facilitating a variety of training scenarios from beginner to advanced users .

## Contents

Product specifications .....	2
Package contents .....	2
Recommended equipment sizes.....	2
Initial set-up information .....	3
List of procedures facilitated by the AirSim Difficult Airway .....	3
Replacement of consumables.....	9
Care and maintenance .....	10
Warranty.....	11

## Product specifications

**Product Code:** DA91100

**AirSim Difficult Airway weight:** Approx. 4kg

**Full shipment weight:** 6kg

**Full shipment dimensions:** 47 x 27 x 34cm

## Package contents

- 1 AirSim Difficult Airway ready-to-use (DA91100)
- 1 AirSim Difficult Airway carrier case (ABAG01)
- 100ml bottle of lubrication (TL001)
- 5 Larynx inserts (NLX050 – 1 supplied on the manikin and 4 spare)
- 1 wraparound neck skin (RSN2005 – supplied on manikin)
- 2 sets of adhesive pads (attachable to suction cups for increased stability if required)

## Recommended equipment sizes

- 7.0-7.5mm ID for nasal intubation
- 8.0-9.0mm ID for oral intubation
- Large / Size 6 for BVM ventilation mask
- Sizes 3-5 for LMA laryngeal masks
- Similar respective sizes for other supraglottic devices

## Initial set-up information

- Gently remove the model from the carrier case
- Secure the manikin to a suitable surface by adjusting the screw on the suction cups (surface must be non-porous to ensure sufficient suction)
- Optional: Adhesive pads are provided with the model for increased stability if required. This is particularly useful when the product is not on an ideal surface for suction cups to be effective. Simply peel the cover from the pad to locate the adhesive area and attach to the suction cups.
- The head can be placed in a neutral or sniffing position by rotating the head, if required for direct laryngoscopy
- Please ensure two lung bags and one stomach bag are attached to the airway and oesophagus respectively
- Spray generous amounts of lubrication provided with the model (TL001) on the airway and equipment prior to use

## List of procedures facilitated by the AirSim Difficult Airway

- Laryngospasm
- Displaced larynx
- Tongue Edema
- Receding / protruding Mandible
- Trismus
- Needle and surgical cricothyroidotomy
- Percutaneous tracheostomy
- Double naso-tracheal intubation
- Bag valve mask (BVM) ventilation techniques
- Full range of supraglottic devices
- Direct laryngoscopy
- Endotracheal tube insertion
- Awake fibre optic examination
- Combi tube insertion
- Video laryngoscopy (including Sellick Manoeuvre)

- Naso-gastric tube insertion techniques

## Airway Features Overview

The AirSim Difficult Airway allows the user to activate features with varying degrees of difficulty quickly and easily, these include Laryngospasm, Tongue Edema and a Displaced Larynx.

The AirSim Difficult Airway has a built-in pump and extendable hose to supply air to each feature. A control toggle situated on the base interface belongs to each of the airway features and is used for activation and deactivation. For specific features, please see below.

### Laryngospasm

1. On the base's interface, switch the laryngospasm control toggle from 'off' to 'on.' This opens the system to allow air to travel to the mechanism.
2. Pull out the pump's hose and attach the hose's spin luer lock to the corresponding luer lock on the base.



3. When connected, use the pump to activate the mechanism - 3 repetitions fill the mechanism fully.
4. Remove the hose and return it to its retracted position.
5. With the hose retracted fully, the feature will remain activated so long as the control toggle remains in the 'on' position.
6. When finished, switch the control toggle to 'off,' this will release the air from the mechanism, and it will return to its inactivated state.

### Displaced Larynx

1. Place the head in your desired position, for best results we recommend placing a pillow under the head or rotating the head into the sniffing position.
2. On the base's interface, switch the Displaced Larynx control toggle from 'off' to 'on.'
3. Pull out the pump's hose and attach the hose's spin luer lock to the corresponding luer lock on the base.



4. When connected, use the pump to activate the mechanism until partially displaced or fully displaced.
5. Remove the hose and return it to its retracted position.
6. With the hose retracted fully, the feature will remain activated as long as the control toggle remains in the 'on' position.
7. When finished, switch the control toggle to 'off,' this will release the air from the mechanism, and it will return to its inactivated state.

### Tongue Edema

The Tongue Edema feature can be adjusted using the 'on' and 'off' toggle.

1. On the base's interface, switch the Tongue Edema control toggle from 'off' to 'on'
2. Pull out the pump's hose and attach the hose's spin luer lock to the corresponding luer lock on the base.



3. When connected, use the pump to activate the mechanism to create a natural tongue, from then further pumps can be used to create a partially or fully inflated Tongue Edema.
4. Remove the hose and return it to its retracted position.
5. With the hose retracted fully, the feature will remain activated as long as the control toggle remains in the 'on' position.
6. When finished, switch the control toggle to 'off' this will release the air from the mechanism, and it will return to its inactivated state.

### Mechanical Features Overview

The AirSim Difficult Airway has the ability to adjust the; Lock jaw, Jaw position and head rotation.

The lockjaw and jaw positions are activated by pin plunger components that have two positions; engaged and disengaged. To disengage the pin plunger, pull the top of the plunger back and twist so that the plungers triangular walls rests on top of the plunger body. To engage, twist the plunger head so that the triangular walls align with the plunger body, the spring will naturally draw the plunger to an engaged position. A click will be heard when the plunger becomes engaged.

### Lockjaw

The lockjaw feature on the model allows the user to lock the jaw in one set position.

1. To activate the Lock Jaw feature, locate the Lock Jaw plunger on the side of the head, twist the plunger head and rotate it, aligning the triangular walls with the plunger body and then release.
2. With the plunger released, push the jaw to a closed position, and audible click will be heard when the plunger engages.
3. To release the lockjaw mechanism, push the jaw to a closed position again, pull the plungers head back and twist until the triangular walls rest on the plunger body.
4. Troubleshooting – if the pin does not engage by itself when pushing the jaw closed, push the jaw closed and the pin plunger at the same time to engage the lock.

### Jaw Position

The AirSim Difficult Airway has the ability to allow the jaw to be free moving, to replicate jaw thrust, but also be able to lock the jaw at multiple distances to create overbite and underbite scenarios.

1. To have the jaw free moving, simply disengage the pin plunger located on the side of the head that reads 'jaw position.' Pull the plungers head back and twist until the triangular walls rest on the plunger body.
2. Move the jaw forward or backward to create the desired overbite or underbite required.

3. Twist the plunger head and rotate it, aligning the triangular walls with the plunger body and then release.
4. An audible click will be heard when the plunger engages with one of the slots and the jaw will be locked out at that position.
5. To move and lock out at a different position, repeat steps 1-4.

### Rotational Lock

The AirSim Difficult Airway as standard allows for head rotation, this can be locked making head rotation impossible. To do this, follow the steps below;

1. Rotate the head forward slightly or lift the head slightly.
2. Locate the rotation lock mechanism on the back of the head.
3. Push the bar down towards the base of the head.
4. The head rotation will then be locked.
5. To release the mechanism, repeat steps 1-3 but this time pull the bar towards the top of the head instead.
6. The head rotation will then be unlocked.

### **Replacement of consumables**

The larynx insert is designed to be replaced for each student to provide a unique training experience. This is a very quick and easy process, perfect for a busy teaching environment.

1. Please ensure the manikin head is placed in a neutral position
2. Remove the wraparound neck skin to provide access to the larynx insert
3. Remove the larynx insert and discard:



4. Align a new insert into position and press into place. Please ensure the ridges at all corners of the insert (yellow areas circled below) are tightly aligned with the larynx insert frame:



### Care and maintenance

Store in clean, dry conditions away from heat and direct sunlight; avoid contact with metals, solvents, oils or greases and strong detergents. When the product is not in use, please store in the black carrier case provided.

Thoroughly wash the AirSim X airway in warm water. Please use warm soapy water or something similar until all visible foreign matter and residue is removed.

Mild detergents or enzymatic cleaning agents may be used on the airway in accordance with the manufacturer's instructions and at the proper dilution. The detergent must not contain skin or mucous membrane irritants.

Please do not use any of the following when cleaning the AirSim product range

- Germicides, disinfectants, or chemical agents such as glutaraldehyde (e.g. Cidex®),
- Ethylene oxide, phenol-based cleaners or iodine-containing cleaners

In response to the recent COVID-19 pandemic, we recommend this additional step to ensure the product is fully sanitised:

Use alcohol spray (minimum 75%) and wipe off. Repeat this for 3-4 times to ensure to kill the virus completely. This method can be used on both the silicone skin and the latex airway.

Care must be taken when removing the unit from a surface if stuck using the adhesive pads for stability. Avoid pulling the unit from the surface, loosen the clear suction screws found at the top of the manikin's head and try to gently remove by sliding a flat object under the adhesive pads to avoid damage to the suction cups.

## Warranty

TruCorp warrants this product to be free from defects in materials and workmanship, ensuring satisfactory performance for a period of one year from the date of delivery. This warranty provides customers with maximum coverage for each unit.

If a product malfunctions and is confirmed to be defective under warranty, TruCorp will repair or replace it at no cost. However, the warranty is void if the unit shows signs of tampering, excessive heat exposure, damage from sharp instruments, improper use, or any conditions beyond TruCorp's control. Consumable items such as wrap-around neck skins and larynx inserts are not covered under warranty and will not be replaced. Damage resulting from misuse is not covered and may incur additional charges.

For full terms and conditions, visit: [TruCorp Warranty Policy](#)

**Please direct all warranty and repair inquiries to:**



**TruCorp Ltd**  
**33 Waringstown Road**  
**Lurgan, Co. Armagh**  
**BT66 7HH**  
**Northern Ireland**  
**[info@trucorp.com](mailto:info@trucorp.com)**  
**Tel: +44 (0) 28 3888 2714**